




# UNIVERSITY OF COLORADO HOSPITAL

ANSCHUTZ MEDICAL CAMPUS

## Collection Container Change Total and Free Phenytoin

Laboratory studies have shown the need to change the current collection container for the phenytoin assays listed below to improve accuracy. On **6/18/2009**, the laboratory collection label will be updated to reflect this change and green tops with gel will no longer be accepted.

Test Mnemonic	Test Name	Current Collection Container	New Collection Container
PHENY TOT	Total Phenytoin	Green Top with Gel	Red Top with No Gel
FREE PHENY	Total and Free Phenytoin	Green Top with Gel	Red Top with No Gel

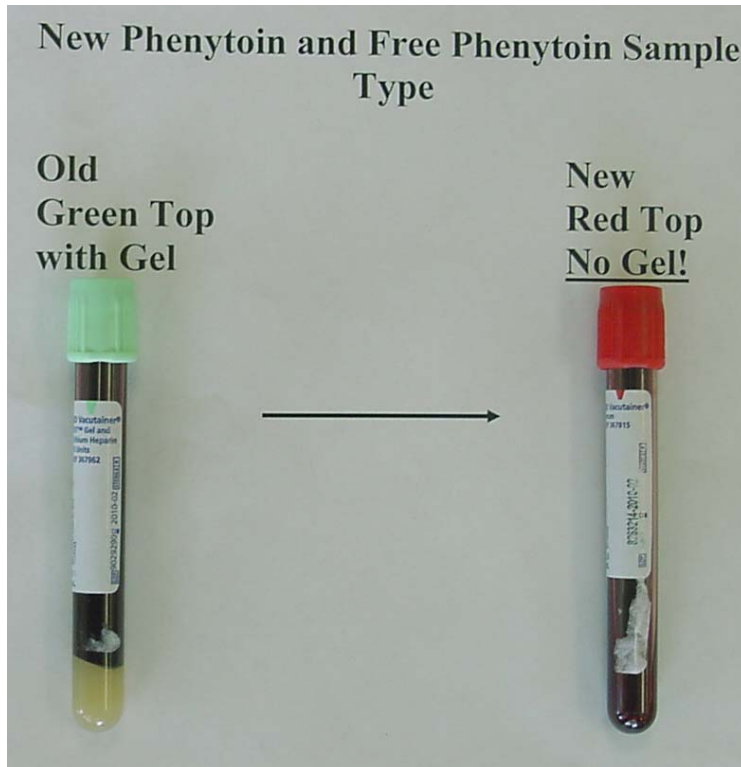

Please call Lorne Holland M.D. at 720-848-7050 if you have any questions or visit our website at <http://www.uch.edu/for-healthcare-professional/Clinical-Laboratory/index.aspx> for additional information. Issued [06-12-2009]

**Clinical Laboratory**  
Medical Director Ronald B. Lepoff, MD